PIKKERTON
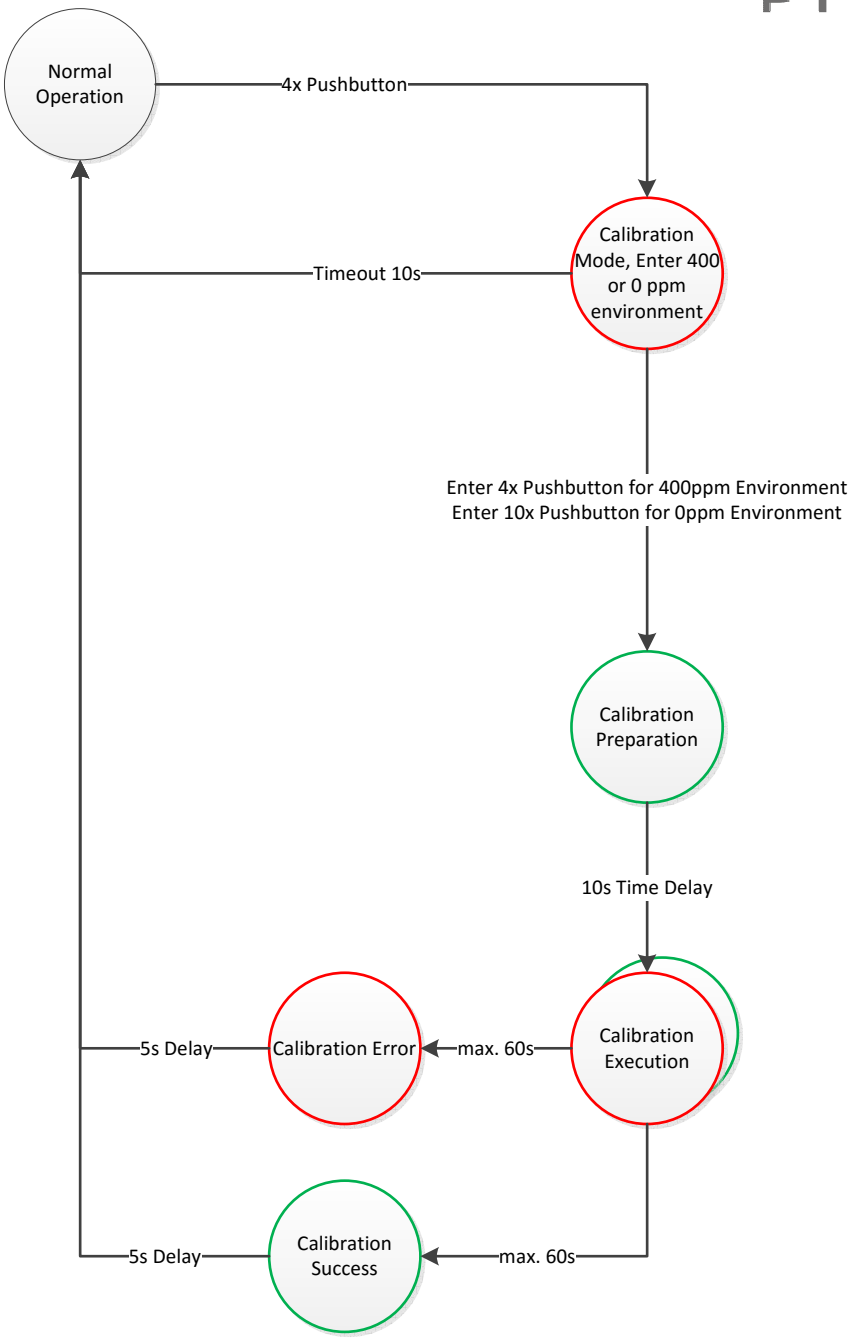
Calibration of xBS Devices with CO2-Sensor
V1.00 / 04.07.2016